



URGENT: FIELD SAFETY NOTICE (Removal)

Specific product codes and lots of:

- Protexis Latex Micro Surgical Gloves

Event-2020-03063

29 July 2020

Attention: Risk Management Director and O.R. Materials Management

Dear Valued Customer:

The purpose of this letter is to advise you that Cardinal Health is voluntarily recalling specific production lots of **Cardinal Health™ PROTEXIS™ Latex Micro Surgical Gloves** that were distributed between June 2019 and July 2020.

Issue Description

This recall is being conducted due to a degradation defect that was found on **Cardinal Health™ PROTEXIS™ Latex Micro Surgical Gloves** that could lead to holes and donning tears at the folding area around the cuffs (Refer to exhibit B for examples of the defect) with the potential risk of infection or cross-patient (clinician) exposure to body fluids. Cardinal Health is not aware of any reports of patient harm.

Cardinal Health is initiating this voluntary recall on the following item codes and lot numbers:

Item Code	Item Description	Lot No.
2D72NT55X	PROTEXIS™ Latex Micro Surgical Gloves Size 5.5	TS19060034, TS19060253, TS19060338, TS19070077, TS19070176, TS19070246, TS19070318, TS19080036, TS19080091, TS19080137, TS19090125, TS19090164, TS19090248, TS19100272, TS19110080, TS19110205, TS19110313, TS19120119, TS19120120, TS20010146, TS20010214, TS20020201, TS20020202, TS20030154, TS20030155, TS20030279, TS20040092, TS20040093, TS20040248
2D72NT60X	PROTEXIS™ Latex Micro Surgical Gloves Size 6.0	TS19060010, TS19060043, TS19060123, TS19060199, TS19060234, TS19070005, TS19070027, TS19070067, TS19070130, TS19070179, TS19070245, TS19070273, TS19080030, TS19080092, TS19080119, TS19080124, TS19080208, TS19080211, TS19080300, TS19080329, TS19090067, TS19090158, TS19090226, TS19090289, TS19100051, TS19100085, TS19100172, TS19100240, TS19100300, TS19110022, TS19110079, TS19110184, TS19110207, TS19110333, TS19120019, TS19120083, TS19120213, TS19120322, TS20010037, TS20010094, TS20010191, TS20010202, TS20010258, TS20010329, TS20020121, TS20020209, TS20030015, TS20030092, TS20030093, TS20030172, TS20030264, TS20030265, TS20030324, TS20040033, TS20040137
2D72NT65X	PROTEXIS™ Latex Micro Surgical Gloves Size 6.5	TS19060012, TS19060037, TS19060064, TS19060118, TS19060140, TS19060158, TS19060235, TS19060257, TS19060303, TS19060340, TS19060393, TS19070019, TS19070068, TS19070084, TS19070138, TS19070185, TS19070231, TS19070247, TS19070297, TS19070317, TS19080022, TS19080040, TS19080051, TS19080093, TS19080110, TS19080128, TS19080134, TS19080209, TS19080239, TS19080258, TS19080269, TS19080326, TS19090044, TS19090058, TS19090104, TS19090200, TS19090212, TS19090262, TS19090295, TS19100043, TS19100099, TS19100138, TS19100173, TS19100221, TS19100280, TS19100310, TS19110023, TS19110058, TS19110076, TS19110083, TS19110150, TS19110211, TS19110349, TS19120020, TS19120073, TS19120084, TS19120233, TS19120323, TS20010017, TS20010048, TS20010072, TS20010109, TS20010166, TS20010193, TS20010265, TS20010306, TS20020024, TS20020098, TS20020108, TS20020149, TS20020247, TS20020248, TS20020262, TS20030066, TS20030078,



CardinalHealth

		TS20030179, TS20030191, TS20030219, TS20030220, TS20030318, TS20030325, TS20040039, TS20040116, TS20040175, TS20040259
2D72NT70X	PROTEXIS™ Latex Micro Surgical Gloves Size 7.0	TS19060002, TS19060036, TS19060115, TS19060216, TS19060238, TS19060258, TS19060274, TS19060339, TS19070029, TS19070092, TS19070108, TS19070180, TS19070285, TS19070320, TS19080035, TS19080037, TS19080064, TS19080138, TS19080140, TS19080186, TS19080210, TS19080257, TS19080271, TS19080320, TS19090004, TS19090054, TS19090126, TS19090149, TS19090263, TS19090266, TS19100058, TS19100107, TS19100186, TS19100253, TS19100308, TS19110026, TS19110038, TS19110068, TS19110090, TS19110157, TS19110225, TS19110324, TS19120005, TS19120056, TS19120109, TS19120141, TS19120161, TS19120162, TS19120257, TS19120258, TS19120299, TS20010002, TS20010051, TS20010085, TS20010129, TS20010184, TS20010246, TS20010247, TS20010305, TS20020074, TS20020075, TS20020140, TS20020146, TS20020223, TS20020227, TS20020284, TS20030094, TS20030165, TS20030166, TS20030227, TS20030228, TS20030299, TS20040045, TS20040046, TS20040130, TS20040197, TS20040139, TS20040367, TS20050112, TS20050158
2D72NT75X	PROTEXIS™ Latex Micro Surgical Gloves Size 7.5	TS19060031, TS19060065, TS19060081, TS19060129, TS19060168, TS19060302, TS19070161, TS19070201, TS19070229, TS19080080, TS19080176, TS19080203, TS19080262, TS19090027, TS19090064, TS19090167, TS19090272, TS19100068, TS19100111, TS19100197, TS19100244, TS19100262, TS19110041, TS19110102, TS19110176, TS19110238, TS19110314, TS19120002, TS19120044, TS19120093, TS19120166, TS19120274, TS19120275, TS19120298, TS20010009, TS20010064, TS20010070, TS20010155, TS20010217, TS20010255, TS20010315, TS20020092, TS20020115, TS20020161, TS20020162, TS20020236, TS20020237, TS20020286, TS20030110, TS20030111, TS20030192, TS20030215, TS20030240, TS20030288, TS20040029, TS20040030, TS20040086, TS20040147, TS20050114, TS20050115
2D72NT80X	PROTEXIS™ Latex Micro Surgical Gloves Size 8.0	TS19060053, TS19060095, TS19060169, TS19060273, TS19060328, TS19060357, TS19070100, TS19080183, TS19080200, TS19080225, TS19080308, TS19090043, TS19090188, TS19090292, TS19100150, TS19100214, TS19100269, TS19100282, TS19110056, TS19110050, TS19110115, TS19110249, TS19110295, TS19110334, TS19120049, TS19120122, TS19120215, TS19120308, TS19120309, TS20010031, TS20010103, TS20050122, TS20050165
2D72NT85X	PROTEXIS™ Latex Micro Surgical Gloves Size 8.5	TS19060044, TS19060122, TS19060189, TS19060356, TS19080111, TS19080184, TS19080227, TS19080321, TS19090008, TS19090127, TS19100079, TS19100220, TS19100271, TS19100309, TS19110075, TS19110069, TS19110109, TS19110148, TS19110285, TS19110331, TS19120038, TS19120118, TS19120214, TS19120316, TS19120317, TS20010036, TS20010093, TS20050031, TS20050139
2D72NT90X	PROTEXIS™ Latex Micro Surgical Gloves Size 9.0	TS19080275, TS19090162, TS19090231, TS19110286, TS19120251, TS20010216, TS20030153

This FSCA affects only the specific combinations of item codes and lots listed above. The applicable regulatory agencies are being notified that Cardinal Health is voluntarily taking this action. We request that you contact Cardinal Health if you have experienced quality problems or adverse events.

Required Actions:

1. **CHECK** all storage and usage locations to confirm whether you have any units of the affected product codes and lot numbers. Exhibit A outlines examples of product labeling and how to identify the affected product. Exhibit B outlines the location of the defect.
2. **Review, complete, sign and return** the enclosed Acknowledgement Form in accordance with the directions on the form.
3. **Return** all affected product or contact your local sales representative to facilitate return of the affected product. Your sales representative will inform you of the product replacement or credit options.



CardinalHealth

4. **Share this letter with others in your facility who need to be made aware of this recall. Contact any other facilities that have been provided with units of affected lot.**
5. **Maintain awareness of this notice until all affected product has been returned to Cardinal Health.**
6. **Keep a copy of this notice with any affected product until returned.**

We apologize for this inconvenience. If you have any questions or concerns, please do not hesitate to contact your local sales representative or local sales office.

Sincerely,

Karl Vahey
Vice President, Manufacturing Quality

EXHIBIT A – Packaging of Affected Product


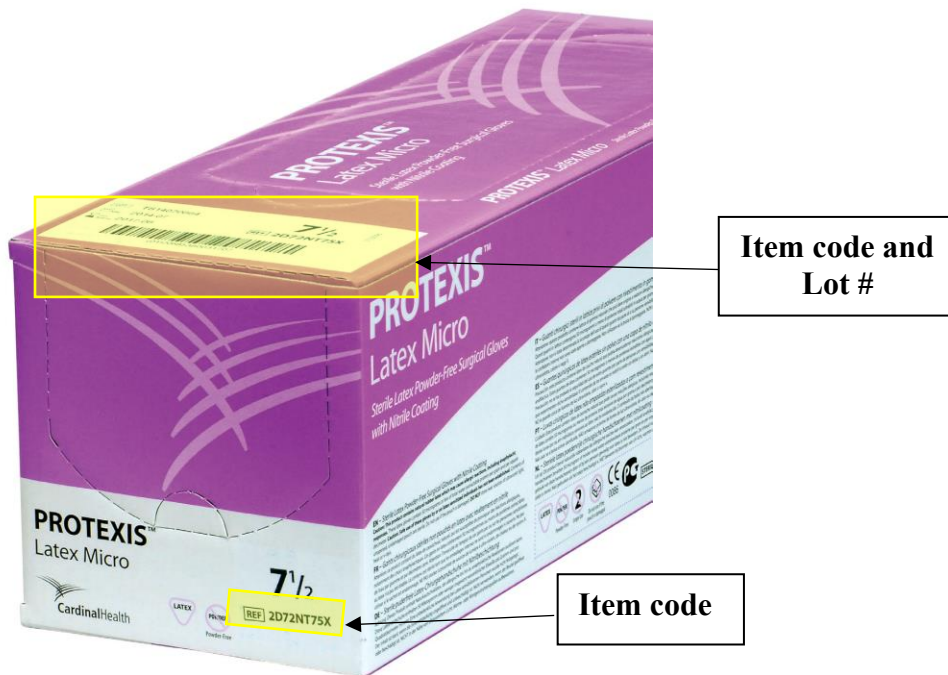


Exhibit B: Examples of the defect

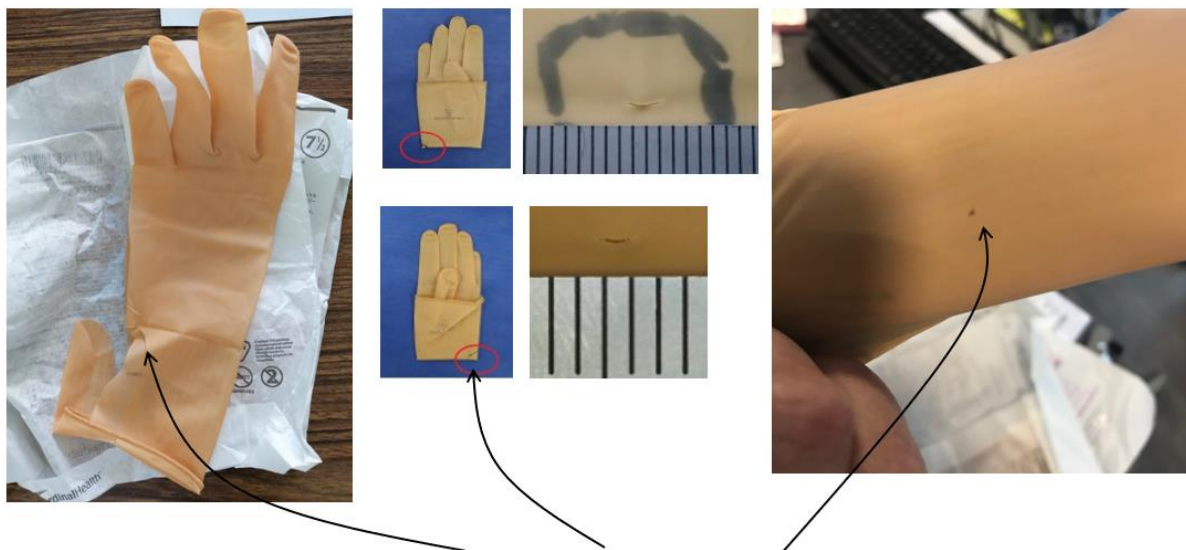

Degradation defect found at cuff (folding area).